

B8

(19) World Intellectual Property Organization  
International Bureau



(43) International Publication Date  
23 January 2003 (23.01.2003)


PCT

(10) International Publication Number  
**WO 03/006085 A2**

- (51) International Patent Classification<sup>7</sup>: **A61M**
- (21) International Application Number: PCT/US02/22068
- (22) International Filing Date: 12 July 2002 (12.07.2002)
- (25) Filing Language: English
- (26) Publication Language: English
- (30) Priority Data:  
09/905,389 13 July 2001 (13.07.2001) US
- (71) Applicant: **RADIANT MEDICAL, INC.** [US/US]; 250 Chesapeake Drive, Redwood City, CA 94063 (US).
- (72) Inventors: **HAMMACK, Amy, L.**; 420 E. Bellevue, Apt. B, San Mateo, CA 94401 (US). **CALLISTER, Jeff, P.**; 955 Cambridge Road, Redwood City, CA 94061 (US). **STUL, Paul, M.**; 235 41st Avenue, San Mateo, CA 94403 (US). **ROTH, Alex, T.**; 1354 Regent Street, Redwood City, CA 94061 (US). **TREMULI, William, S.**; 399 Mindinao Drive, Redwood City, CA 94065 (US).
- (74) Agent: **BUYAN, Robert, D.**; Stout, Uxa, Buyan & Mullins LLP, 4 Venture, Suite 300, Irvine, CA 92618 (US).
- (81) Designated States (*national*): AE, AG, AL, AM, AT, AU, AZ, BA, BB, BG, BR, BY, BZ, CA, CH, CN, CO, CR, CU, CZ, DE, DK, DM, DZ, EC, EE, ES, FI, GB, GD, GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MA, MD, MG, MK, MN, MW, MX, MZ, NO, NZ, OM, PH, PL, PT, RO, RU, SD, SE, SG, SI, SK, SL, TJ, TM, TN, TR, TT, TZ, UA, UG, UZ, VN, YU, ZA, ZM, ZW.
- (84) Designated States (*regional*): ARIPO patent (GH, GM, KE, LS, MW, MZ, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European patent (AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE, SK, TR), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).
- Published:**  
— without international search report and to be republished upon receipt of that report

[Continued on next page]

(54) Title: CATHETER SYSTEM WITH ON-BOARD TEMPERATURE PROBE

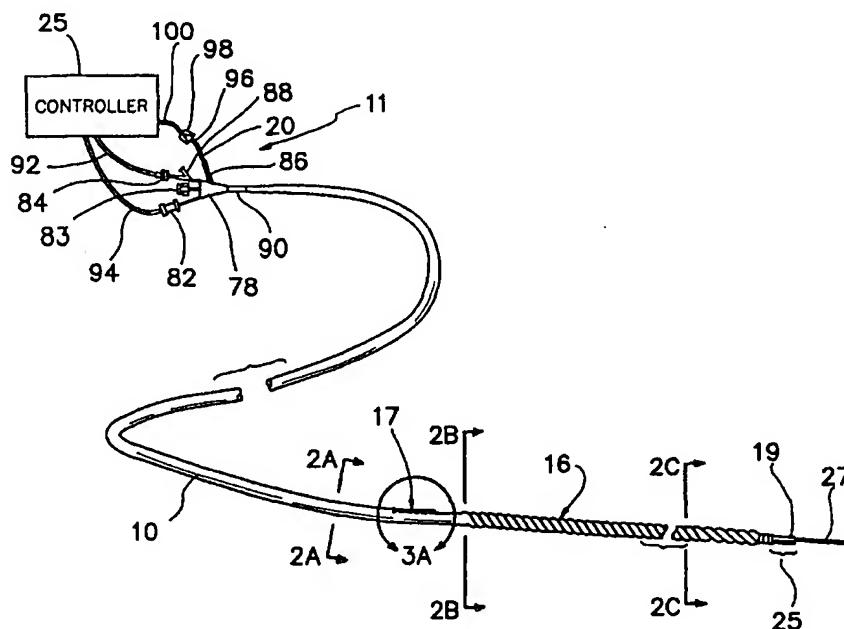

(57) Abstract: A catheter system for controlling the body temperature of a patient by modifying the temperature of blood flowing within a blood vessel of the patient. The catheter system comprises a catheter body having a heat exchange region in contact with the blood; and a temperature probe having a distal end that extends from the catheter body, thereby monitoring the temperature of blood flowing within the blood vessel.



WO 03/006085 A2



---

*For two-letter codes and other abbreviations, refer to the "Guidance Notes on Codes and Abbreviations" appearing at the beginning of each regular issue of the PCT Gazette.*

# **CATHETER SYSTEM**

## **WITH ON-BOARD TEMPERATURE PROBE**

### **BACKGROUND OF THE INVENTION**

#### **1. Field of the Invention**

The present invention relates generally to medical devices and a method of using them for selectively affecting the temperature of a patient's body, or a portion of the patient's body, and more particularly, to a temperature control catheter system including an on-board temperature probe and a method of use thereof.

#### **2. Description of the Prior Art**

Under ordinary circumstances, the thermoregulatory system of the human body maintains a near constant temperature of about 37° C (98.6° F), a temperature generally referred to as normothermia. For various reasons, however, a person may develop a body temperature that is below normothermia, a condition known as hypothermia, or a temperature that is above normothermia, a condition known as hyperthermia. Accidental hypothermia and hyperthermia are generally harmful, and if severe, the patient is generally treated to reverse the condition and return the patient to normothermia. Accidental hypothermia significant enough to require treatment may occur in patients exposed to overwhelming cold stress in the environment or whose thermoregulatory ability has been lessened due to injury, illness or anesthesia. For example, this type of hypothermia sometimes occurs in patients suffering from trauma or as a complication in patients undergoing surgery.

However, in certain other situations hyperthermia and particularly hypothermia may be desirable and may even be intentionally induced. For example, hypothermia is generally recognized as being neuroprotective, and may, therefore, be induced in conjunction with cardiac surgery where there is an interruption or decrease of cardiac

output of oxygenated blood, treatments for ischemic or hemorrhagic stroke, blood deprivation caused by cardiac arrest, intracerebral or intracranial hemorrhage, head and spinal trauma, brain or spinal surgery, or any other situation where there is danger to neural tissue because of ischemia, increased intracranial pressure, edema or other similar processes.

5

Other examples where hypothermia may be neuroprotective include periods of cardiac arrest in myocardial infarction and heart surgery, neurosurgical procedures such as aneurysm repair surgeries, endovascular aneurysm repair procedures, spinal surgeries, procedures where the patient is at risk for brain, cardiac or spinal ischemia such as beating heart by-pass surgery or any surgery where the blood supply to the heart, brain or spinal cord may be temporarily interrupted.

Hypothermia has also been found to be protective of cardiac muscle tissue when that muscle tissue is at risk, for example during or after a myocardial infarct (MI), or during cardiac surgery, cardiac arrest, or other situations where there is deprivation of the normal blood supply to the cardiac tissue. Indeed the tissue protective nature of hypothermia in general is recognized in a vast array of situations.

Simple surface methods for cooling such as cooling blankets, immersion in cold water or ice baths, or alcohol rubs are generally ineffective for inducing hypothermia. The body's normal thermoregulatory responses such as vasoconstriction of capillary beds at the surface of the body and arterio-venous shunting of blood away from the skin act to render such cooling methods ineffective. Further, if the body temperature drops sufficiently below normothermia, usually at about 35.5°C, the body begins to shiver as a thermoregulatory response to generate additional metabolic heat and fight the induction of hypothermia. This may increase the generation of metabolic heat by 200 - 500 % and generally makes induction of hypothermia in an awake patient impossible by surface cooling alone. Further, the shivering itself is so uncomfortable and exhausting for the patient that this is altogether unacceptable for an awake patient. Only if the patient is paralyzed, which necessitates the patient be intubated for breathing and be placed under general anesthesia can the patient be subjected to significant surface cooling. Even under these conditions, surface cooling which necessitates cooling through the skin and surface fat layers and the use of generally low

power surface cooling devices, is too slow and inefficient to be an acceptable means of inducing therapeutic hypothermia.

Furthermore, if control of the patient's temperature is desired so as to attain and maintain a target temperature (sometimes but not always normothermia), or to reverse hypothermia and re-warm the patient at a predetermined rate, surface cooling and warming far too slow and inefficient to give the required level of prompt and precise change in the patient's core temperature to allow these methods to control the patient's thermal condition.

A patient's temperature may be controlled by a very invasive method of adding heat to or removing heat from a patient's blood, particularly in the case of heart surgery. Blood is removed from a patient, circulated through a heart-lung by-pass system, and reintroduced into the patient's body. The equipment generally has a temperature control unit that heats or cools the blood as it is circulated out of the patient before it is reintroduced into the patient. Because a large volume of blood is circulated through the machine in a short time, this by-pass method may be both fast and effective in changing the patient's core temperature and in controlling that temperature, but has the disadvantages of requiring a very invasive medical procedure which requires the use of complex equipment, a team of highly skilled operators, is generally only available in a surgical setting where the patient has undergone a thoracotomy (had its chest split and opened), and involves mechanical pumping of a huge quantity of the patient's blood and channeling that blood through various external lines and conduits, all of which is generally very destructive of the blood tissue resulting in the cytotoxic and thrombolytic problems. In fact, most surgeons using such by pass machinery tend to avoid its use for longer than four hours, much less if at all possible, which is an inadequate period of time for treatment of some conditions such as stroke.

One method for adding or removing heat from a patient by adding or removing heat from the patient's blood that does not involve pumping the blood with an external, mechanical pump is by placing a heat exchange catheter in the bloodstream of a patient and exchanging heat through the catheter. This endovascular temperature management (ETM) technique was described in U.S. Patent No. 5,486,208 to Ginsburg, the complete disclosure of which is incorporated herein by reference. The Ginsburg patent discloses a method of controlling the temperature of a body by adding or removing heat to the blood by inserting a heat exchange catheter having a heat exchange region into the vascular

system and exchanging heat between the heat exchange region and the blood to affect the temperature of a patient. One method disclosed for doing so includes inserting a catheter having a heat exchange region comprising a balloon into the vasculature of a patient and circulating warm or cold heat exchange fluid through the balloon while the balloon is in  
5 contact with the blood.

In successful ETM, in addition to fast and precise changes in a patient's body temperature, fast and precise control over a patient's thermal condition is very important whether the patient is being cooled, warmed, or maintained at a constant temperature. A  
10 general apparatus and method of ETM control based on temperature management responsive to feedback from temperature probes in or on the patient is disclosed in U.S. Patent No. 6,149,673 to Ginsburg, the complete disclosure of which is incorporated herein by reference. A similar method is described in PCT publication WO 01/10494 to Radiant Medical Inc., the complete disclosure of which is also incorporated herein by reference. In such methods, a  
15 signal representing the temperature of a target tissue, which as mentioned may be the core body temperature, is directed to a controller from a temperature probe inserted on or in the patient, and the controller then controls the exchange of heat between the heat exchange catheter and the patient's blood flowing past that catheter. That in turn controls the temperature of the patient. With such a method, it is clear that precise, accurate and  
20 convenient control is dependent to a large extent on the precise, accurate, and convenient temperature measurement of the temperature of the target tissue (which may be the core body temperature) and thus dependent on a precise, accurate and convenient temperature probe.

Currently, the patient's temperature may be measured by any one or several  
25 generally available temperature probes. These include, for example, skin temperature probes, tympanic probes that may be placed in the ear canal and perhaps even in physical contact with the ear drum, esophageal probes including nasoesophageal probes, rectal probes, bladder probes, temperature sensors placed on an insertion sheath, and temperature probes that may be inserted by needle directly into the target tissue. Each of these techniques, however,  
30 suffers from significant shortcomings.

Some probes may not give an accurate temperature of the target tissue and therefore may not provide the information necessary for controlling the ETM procedure. For example, if the target is the core temperature of the patient, a skin temperature is generally

not an accurate representation of the core temperature; if cardiac muscle is the target tissue, a bladder probe might not be sufficiently accurate. The probe might not be sufficiently responsive to changes in temperature to provide a current temperature of the target temperature. For example, a rectal temperature probe is generally very slow to respond to temperature changes in the core, and thus if the controller is receiving its temperature signal from a rectal probe, it might not be able to respond with sufficient speed and precision to changes in the core temperature. Bladder temperature probes also tend to suffer from this problem. Some probes are awkward and too difficult to use. For example, tympanic probes are difficult to place and tend to fall out and thus not provide an accurate temperature measure. Where a temperature probe is controlling an ETM procedure and thus in the patient at the same time as an ETM catheter, it may reflect the temperature of the ETM catheter rather than the target tissue if the probe is located too close to the catheter. Probes placed on the insertion sheath, for example, may tend to be unduly influenced by the heat exchange catheter placed through the sheath. Other probes may measure the temperature of the target tissue, but have other disadvantages that make their use undesirable. For example, needle temperature probes that are stuck directly into the target tissue, of course, measure the temperature of the target tissue, but are invasive and require the patient suffer an additional needle stick. They are also dependent on accurate placement in the first instance which may be a difficult and highly skilled procedure, and require that they do not move after placement, requiring constant monitoring and taping or the like which may be obtrusive and awkward.

If redundancy is important for safety, as it usually is in a controlled ETM procedure, all of the above devices would generally require the placement of two probes. This may require two probes placed in different locations that may reflect different temperature profiles, a very real problem for controlling ETM. It may require that two probes be attached together, which makes the probes large and often clumsy to use.

Very importantly, when used to control an ETM procedure, all of the above require a device (the probe) in addition to the ETM catheter already being inserted into the patient's body. These are generally separately placed requiring an additional procedural step, are often quite distal to the insertion site of the catheter but must still be attached to the controller that is attached to the ETM catheter. This may greatly complicate what may already be a crowded operating room or other area and add undesirable complexity to the procedure.

For ETM to accurately control the temperature of a target tissue, it is important that the temperature measured by the probe provides current and accurate measurement of the temperature of the target tissue and responds quickly to changes in temperature of the target temperature. This is not always the case with the probes mentioned above. If the controller precisely and rapidly responds to the temperature feedback to control the temperature of the target tissue, for example if the patient's temperature is being increased at a very precise rate of, for example, 0.2 °C per hour, the controller must act to add heat when the temperature is not increasing fast enough, remove heat if the body is adding metabolic heat so fast that it would result in rewarming too fast, or maintain the temperature of the heat exchange catheter the same as the blood if the patient's temperature is increasing at exactly the correct rate. The systems described in the publications incorporated above may be capable of such precision, but rely on temperature information from the temperature probes that is current and accurate.

Temperature probes placed directly in the bloodstream in one of the great vessels such as the inferior vena cava (IVC) generally accurately reflect the core body temperature which is also generally the temperature of the brain or heart tissue, currently the two most common target tissues for ETM, but if the probe is placed some distance from the heat exchange catheter such placement usually involves an additional incision or puncture into the vasculature, and if the probe is placed in the same general vicinity as the heat exchange catheter, there is a likelihood that the temperature reading will be unacceptably influenced by the heat exchange region on the catheter or the temperature of the catheter shaft and thus not represent the temperature of the target tissue sufficiently to serve as a control temperature for the system.

Further, when the temperature probe is placed in the vasculature in general, the distal tip of the probe which generally houses the temperature sensor itself may come into contact with the wall of the vessel. In such a case, the temperature that is sensed will be that of the vessel wall and not of the blood. While these two temperatures may often be the same, there will be occasions where they may be unacceptably different. Furthermore, the distal tip of such a probe must be designed so that it will not be traumatic to the vessel wall. It would be best, of course, if contact with the vessel wall could be avoided altogether.



When any device is inserted into a patient, the physician generally would prefer to make as small an incision or puncture as possible. Thus where a probe is inserted into the bloodstream, a low profile is generally preferable. If the probe is attached or otherwise associated with another device that is being inserted into a patient, a means to keep the overall profile to the device being inserted would be desirable.

Accordingly, it would be helpful to have a temperature probe that was easy to place in conjunction with an ETM procedure.

It would also be helpful to have a temperature probe that precisely and accurately measured a relevant tissue temperature for ETM.

It would also be helpful to have a temperature probe that rapidly responded to changes in temperature in a target tissue.

It would also be helpful to have a temperature probe that did not create additional crowd the treatment area during treatment by ETM.

It would also be helpful to have a temperature probe that did not require additional punctures or incisions in a patient undergoing ETM.

It would also be helpful to have a temperature probe that had a deployed and an undeployed configuration.

Accordingly, it would be helpful to have a temperature probe located in the blood stream at a location close to the heat exchange catheter to accurately measure the temperature of the blood but not be unduly influenced by the temperature of the heat exchange catheter.

It would be helpful to have a temperature probe that had a plurality of temperature sensors for redundancy and safety.

It would be helpful to have a temperature probe that had an atraumatic distal tip.

It would be helpful to have a temperature probe that could be advantageously inserted into the vasculature of a patient undergoing EMT without the need of a second incision or puncture.

5

It would be helpful to have a temperature probe that was an on-board temperature probe.

It would be helpful to have a temperature probe that had a deployed and an undeployed position, wherein the operator could move the probe between the deployed and the undeployed configuration.

Furthermore, it would be helpful to have a system and method that ensure that the temperature reading provided at the heat exchange catheter is accurate in order to ensure appropriate operation of the heat exchange catheter.

15

## SUMMARY OF THE INVENTION

The present invention provides a catheter that includes an on-board temperature sensor.

20

In one aspect of the invention, the present invention provides a catheter system for sensing the temperature of a patient. The catheter system includes a catheter having a shaft, a heat exchange region and a temperature probe lumen. The temperature probe lumen defines an aperture that is located proximal of the heat exchange region. A deployable temperature probe is provided that includes a temperature sensor and a signal carrying mechanism that extends from the sensor to a location outside of the patient. The temperature probe has an undeployed configuration and a deployed configuration and is movable between the undeployed and deployed configurations. When the temperature probe is in the deployed configuration, the temperature sensor is located further from the shaft than when the temperature probe is in the undeployed configuration. The temperature sensor generates a signal representing a sensed temperature and the signal carrying mechanism transmits the signal from the temperature sensor to the location outside the patient.

30

In accordance with one aspect of the present invention, the distal end of the movable temperature probe comprises a thermistor.

5 In accordance with a further aspect of the present invention, the distal end of the temperature control lumen includes a ramp coupled to the opening.

In accordance with yet another aspect of the present invention, the opening is in the form of a flat slot and a portion of the temperature probe is flat.

10 In accordance with yet another aspect of the present invention, the movable temperature probe includes an atraumatic tip at the distal end portion.

15 In accordance with yet another aspect of the present invention, the movable temperature probe comprises a shape memory metal such as nickel-titanium alloy (nitinol) at a tip portion of the distal end portion.

The present invention also provides a temperature probe that includes two temperature sensors.

20 The present invention also provides a temperature probe having a heat memory shaped distal portion containing a temperature sensor wherein the distal portion of the probe assumes a shape when warmed by blood flow that positions the temperature sensor away from the catheter shaft;

25 The present invention also provides a catheter shaft having channels for the flow of heat exchange fluid and a temperature sensor that is positioned by the inflation of a balloon on the catheter shaft at a location away from the heat exchange fluid channels;

30 The present invention also provides a catheter system having a temperature probe with a temperature sensor in its distal portion, the temperature sensor is deployable to locate the temperature sensor away from the catheter shaft;

The present invention also provides a catheter system with a temperature sensor that has a first configuration having one profile for insertion, and a second

configuration that has a greater profile wherein the temperature sensor is located farther away from the catheter shaft in the second configuration than in the first configuration;

The present invention also provides a method of monitoring the body  
5 temperature of a patient by monitoring the temperature of blood flowing within a blood vessel of the patient. The method includes advancing a catheter body comprising a temperature control lumen coupled to the catheter shaft wherein the temperature control lumen includes an opening defined at a distal end of the catheter, into the patient's blood vessel such that the opening is in contact with the patient's blood. The method further  
10 includes moving a temperature probe within the temperature control lumen such that a distal end portion of the movable temperature probe protrudes through the opening into the blood flowing within the blood vessel.

The present invention thus provides catheters and methods for inducing or  
15 treating hypothermia or hyperthermia by inserting a catheter body into a blood vessel of the patient, moving a temperature probe into the blood stream within the blood vessel and selectively transferring heat either to or from the blood flowing through the vessel while monitoring the temperature of the blood stream. It enhances the ability to monitor the temperature of the blood stream, thereby enhancing both the ability to induce or treat  
20 hypothermia or hyperthermia and the ability to rapidly and precisely control the body temperature of the patient.

Other features and advantages of the present invention will be understood  
upon reading and understanding the detailed description of preferred exemplary embodiments  
25 found herein below, in conjunction with reference to the drawings, in which like numerals represent like elements.

### BRIEF DESCRIPTION OF THE DRAWINGS

30 Figure 1 is a perspective view of a catheter system in accordance with the present invention;

Figure 2A is a sectional view of the catheter illustrated in Figure 1 taken along the line 2A-2A;

Figure 2B is a sectional view of the catheter illustrated in Figure 1 taken along the line 2B-2B;

5                    Figure 2C is a cross section of the balloon portion of the catheter taken along the lines 2C-2C in Figure 1;

                    Figure 3A is a sectional view of the catheter illustrated in Figure 1 of the portion of the catheter of Figure 1 contained in circle 3A-3A;  
10

                    Figure 3B is an sectional side view of a distal end portion of a temperature probe lumen in accordance with the present invention;

                    Figure 4 is a sectional side view of a distal end portion of a temperature probe lumen in accordance with an alternative embodiment of the present invention; and  
15

                    Figure 5 is a sectional side view of a distal end portion of a temperature probe lumen in accordance with an alternative embodiment of the present invention; and

20                    Figure 6 is a sectional side view of a distal end portion of a temperature probe lumen in accordance with an alternative embodiment of the present invention.

                    Figure 7 is an elevational view of the cable and connector of the invention;

25                    Figure 8A is a sectional side view of a distal end portion of a catheter system of an alternative embodiment of the present invention with the probe shown in a deployed state;

                    Figure 8B is a sectional side view of a distal end portion of a temperature probe in accordance with an alternative embodiment of the present invention with the probe shown in a collapsed state;  
30

Figure 9A is a sectional side view of a distal end portion of a temperature probe in accordance with an alternative embodiment of the present invention with the probe shown in an undeployed state;

5           Figure 9B is a sectional side view of a distal end portion of a temperature probe in accordance with an alternative embodiment of the present invention with the probe shown in a deployed state;

10           Figure 10A is a sectional side view of a distal end portion of a temperature probe in accordance with an alternative embodiment of the present invention with the probe shown in an undeployed state;

15           Figure 10B is a sectional side view of a distal end portion of a temperature probe in accordance with an alternative embodiment of the present invention with the probe shown in a deployed state;

20           Figure 11A is a sectional side view of a distal portion of a temperature probe in accordance with an alternative embodiment of the present invention with the probe shown in an undeployed state;

            Figure 11B is a sectional side view of a distal portion of a temperature probe in accordance with an alternative embodiment of the present invention with the probe shown in a deployed state;

25           Figure 12A is a sectional side view of a distal end portion of a temperature probe in accordance with an alternative embodiment of the present invention with the probe shown in an undeployed state;

30           Figure 12B is a sectional side view of a distal end portion of a temperature probe in accordance with an alternative embodiment of the present invention with the probe shown in a deployed state;

Figure 13A is a sectional side view of a distal end portion of a temperature probe in accordance with an alternative embodiment of the present invention with the probe shown in an undeployed state;

5                   Figure 13B is a sectional side view of a distal end portion of a temperature probe in accordance with an alternative embodiment of the present invention with the probe shown in a deployed state;

                  Figure 14 is a cross section of the catheter system of the invention taken along  
10   the line 14-14 in Figure 13B;

                  Figure 15A a sectional side view of a distal end portion of a catheter system of the present invention;

15                   Figure 15B is a sectional side view of a distal end portion of a catheter system in accordance with an alternative embodiment of the present invention;

                  Figure 16A is a sectional side view of a distal end portion of a temperature probe in accordance with an alternative embodiment of the present invention with the probe  
20   shown in an unadvanced state;

                  Figure 16B is a sectional side view of a distal end portion of a temperature probe in accordance with an alternative embodiment of the present invention with the probe  
25   shown in an advanced state;

                  Figure 17A is a sectional side view of a distal end portion of a temperature probe in accordance with an alternative embodiment of the present invention with the probe shown in an undeployed state;

30                   Figure 17B is a sectional side view of a distal end portion of a temperature probe in accordance with an alternative embodiment of the present invention with the probe shown in a deployed state;

Figure 18A is an elevational view of the proximal end of a catheter system of Figure 17A where the distal end of the probe is undeployed; and

Figure 18B is an elevational view of the proximal end of a catheter system of Figure 17B with the distal end of the probe deployed.

#### DESCRIPTION OF SPECIFIC EXEMPLARY EMBODIMENTS

Referring to Figure 1, a heat exchange catheter system that includes a catheter body 10 is illustrated. Catheter body 10 may comprise any type of heat exchange catheter. Numerous suitable examples of heat exchange catheter systems which may comprise the present catheter body 10 are found in various U. S. Patents, and the present invention may be adapted for use with a wide variety of such different temperature regulating catheter systems. For example, in accordance with the present invention, the catheter system used may comprise a catheter system adapted for warming the body fluid passing thereover (for example, a system having an electric heater disposed therein, or a catheter with a heat exchange region thereon which is warmed by circulating warm heat exchange fluid therethrough). In addition, the catheter system used may comprise a catheter system adapted for cooling the body fluid passing thereover (for example, a catheter with a heat exchange region such as a heat exchange balloon or the like thereon, which heat exchange region is placed in the blood stream and cooled by pumping a cooled fluid flow therethrough). Furthermore, those skilled in the art will understand that even non-heat exchange catheters may be used with the present invention if a catheter having an on-board deployable temperature probe is desirable.

In the embodiment of the invention illustrated in Figure 1, catheter body or shaft 10 includes a proximal end portion 11 in the form of a Y adaptor, a heat exchange region 16 on the distal portion of the catheter in the form of a helically wound multi-lobed balloon, a temperature probe exit region 17 as illustrated in Figure 3A, and a distal end 19 having a soft, atraumatic tip 25.

The heat exchange region 16 is heated or cooled by the flow of a heat exchange liquid therethrough. Referring to Figure 2A, the shaft 10 has four lumens therein



proximal of the temperature probe exit region 17, and three lumens therein immediately distal of that region. Proximal of that region, the shaft includes an inflow lumen 12, an outflow lumen 13, a guidewire lumen 14 and a temperature probe lumen 15. The transition between the four lumen (Figure 2A) and three lumen (Figure 2B) catheter tubing may be made by merely skiving off the top portion of the tube, or may result from joining a three lumen extrusion to a four lumen extrusion using extension tubes between the three lumens that remain in the distal shaft and placing an external jacket around that joined length of catheter shaft made of the two different extrusions. The jacket may be heat shrunk or heat welded around the tubes to secure the joint. Outflow lumen 13 is fluidly connected between outflow connector 84 and outflow lumens 58, 60, 62. Inflow lumen is fluidly connected between inflow connector 82 and balloon inflow lumen 64. A complete description of heat transfer catheters similar to that described here is included in U.S. Patent No. 6,231,594 B1 owned by applicant's assignee and incorporated herein in full, and U.S. application number 09/777,612.

15

The proximal end of the catheter of the invention terminates in a Y adaptor 78 which is attached to an outflow connector 84, an inflow connector 82, a guide wire lumen terminus 83, a temperature probe lumen terminus 86, and an aspiration valve 88. A short length of strain relief tubing 90 may be placed over the catheter at the location where it attaches to the Y adaptor. The outflow connector may fluidly connect the outflow lumen 13 to an outflow line 92 carrying heat exchange fluid between the outflow lumen and the controller 25. The inflow connector fluidly connects the inflow lumen of the catheter 12 to an inflow line 94 that carries heat exchange fluid from the controller to the inflow lumen. The inflow connector 84 may be closed, or the inflow line 94 closed with a clamp (not shown), and the heat exchange fluid in the balloon withdrawn through the aspiration valve 88 when it is desired to collapse the balloon, for example when the catheter is to be withdrawn from within the vasculature of a patient. The guide wire lumen terminus provides access from the Y adaptor to the guide wire lumen 14 that extends entirely through the catheter for insertion of a guide wire 27 therethrough. The guidewire lumen also functions as a working lumen for the injection of drugs, thrombolytics, or other substances from outside the body to a location distal to the catheter, or for sensing the pressure of the blood stream distal of the catheter. It is also possible to insert other devices through the lumen, for example a temperature sensor for sensing the temperature distal of the heat exchange balloon, an angioplasty catheter for treating the patient at a location distal of the balloon, an angiojet type

device or any similar type device for treatment distal of the balloon. In fact, it is possible if a temperature is sensed proximal of the balloon, and another temperature is sensed distal of the balloon, and the amount of energy emitted or absorbed by the balloon is determined, to determine blood flow. Another depiction of the proximal portion of the catheter is shown in Figure 7.

The proximal portion of the temperature probe 20 exits the catheter from the temperature probe lumen terminus 86. The proximal end terminates in an appropriate plug, for example a plastic clip type plug 96. That plug, in turn attaches to a clip type jack 98 reminiscent of the type of plastic clip attachments common in telephones and similar devices. This plug to jack attachment connects the temperature probe electrically to the temperature probe cable 100 which in turn is connected to the controller. This provides for temperature signals generated by the temperature probe to be transmitted to the controller so that the controller may control the heating and cooling of the patient as effected by the catheter based on temperature feed back from the patient as described in U.S. Patent Nos. 6,149,673 and 6,149,676 incorporated herein in full. The controller may control the exchange of heat between the blood and the heat exchange region by altering the temperature of the heat exchange fluid or by altering the flow rate of the heat exchange fluid through the catheter, or some combination thereof, in response to the temperature signal. One controller suitable for receiving temperature signals generated by the present invention and using said signals to control the transfer of heat from a patient is described in U.S. Patent Application 09/707,257 incorporated herein in full.

A temperature probe 20 is included and is movable within temperature probe lumen 15. As can be seen in Figures 3b, 4, 5 and 6, the temperature probe preferably includes temperature sensor such as a thermistor 21 at its distal end portion 22. Other temperature sensors may be employed, for example a thermocouple, light probes capable of sensing temperature, infra red sensors, or similar device, as long as the sensor is able to sense the temperature of a specified tissue and generate a signal representing that temperature that may subsequently be transmitted to a controller for controlling the heat exchange of a heat exchange catheter or for some other desired purpose. In the example as shown in this embodiment, the temperature sensor is a thermistor, the temperature sensed is that of the blood surrounding the thermistor, and the signal generated is an electrical signal representing

that temperature Thermistors have been found to be advantageous because they can be made very small and because they can be made sufficiently accurate.

At least a portion 23 of the temperature probe adjacent its distal end portion generally comprises insulating materials. A coating of plastic 106, as in encasing the signal wires 102, 104 within a plastic tube, may be sufficient. It is important that the wires that carry the electric signal from the thermistor be sufficiently insulated that they do not conduct the temperature of the heat exchange catheter to the thermistor and thereby significantly influence the temperature sensed by the thermistor.

For safety reasons, it is generally preferable that there be redundancy in the temperature sensors. For example, the distal portion of the temperature probe may contain two thermistors each of which has independent connector wires that extend down the probe to the connection 96/98 and thus to the controller. The controller is generally programmed so that if the two signals do not correspond to each other within some predetermined range, the controller responds appropriately. For example, it may sound an alarm; it may flash a warning on a user interface if it has one; it may cease to provide hot or cold heat exchange fluid to the catheter, or any combination including all of the above. While this redundancy will generally not be repeated as to each embodiment described below, it is to be understood that such redundancy may be a feature incorporated into each embodiment. Furthermore, the redundancy may be accomplished by incorporating two or more sensors in each probe, or by incorporating more than one embodiment of the probe in a particular catheter.

Figures 2A, 2B illustrate cross sections of the catheter depicting the portion of the catheter shaft containing the temperature probe lumen. The inner diameter of temperature probe lumen 15 is generally in a range of 0.020" to 0.035". Preferably, the inner-diameter of the temperature probe lumen is about 0.030 and may not be round, depending on the extrusion. The temperature probe along its length is configured to move through the lumen, for example, the probe may comprise a tube with thermistors in it near the distal end and wires for transmitting a signal from the thermistors contained within the tube. The tube may have, for example an outer diameter of about 0.025 or less. As described below, the diameter of the probe along its length may vary. For example, a portion may be flat for alignment with a flat exit ramp; a portion may have a slightly larger diameter so that it cannot be entirely withdrawn, or the like. If the probe is of the type that is moved within the

temperature probe lumen, the probe, the lumen, or both may be constructed of material that slides easily against the other such as PTFE (Teflon™) or FEP.

Figure 4 illustrates a slot 30 at the distal end portion of the temperature control lumen. The slot is provided to allow thermistor 21 of temperature probe 20 to protrude from the catheter in order that the thermistor may be advanced away from the catheter shaft and into the blood stream after the catheter is inserted into a subject's blood vessel. As can be seen in Figure 4, the thermistor preferably curls into a substantially J-shape so that it moves away from the catheter and the any temperature effects of the heat exchange catheter, thus allowing the thermistor to obtain a more accurate measurement of the temperature of blood flow of the subject. Preferably, the tip of the temperature probe containing the thermistor moves at least 1.8 mm away from the catheter. The temperature control catheter generally contains a flow of heat exchange fluid at a temperature different than the blood temperature of the patient, and it has been found that if a temperature is sensed by the thermistor at a distance greater than 1.8 mm from the shaft of the catheter, it generally accurately represents the temperature of the blood flowing within the vessel and is not unduly influenced by the temperature of the catheter shaft. It may be possible to advance the probe too far, however. For example, if the catheter is in a vessel and the sensor is too far away from the shaft, the sensor in may impact on the vessel wall. Likewise, if the sensor portion of the temperature probe is extended too far out of the temperature probe lumen, it may prolapse back onto the catheter shaft and the temperature sensed may be significantly influenced by the temperature of the catheter shaft.

The location of the distal exit opening in the temperature probe lumen along the length of the catheter is also important. When the catheter is used for whole body cooling in the inferior vena (IVC) the catheter is generally inserted through an introducer sheath into the femoral vein and advanced so that the balloon is located entirely in the IVC. So that the cooling may be maximized, it is desirable that the balloon occupy as much as possible of the length of the IVC. That means that the shaft of the catheter is located to a large extent in the femoral vein, a much smaller vein than the IVC. In fact the shaft extends all the way back through the introducer sheath. The blood in the introducer sheath tends to flow very little if at all, and therefore to be greatly influenced by the temperature of the catheter shaft. Thus it is desirable that the temperature sensed be that of the blood in the IVC and not in the femoral vein or in the introducer sheath. Yet if the sensor is too close to the balloon, the effect heat

exchange region, it is likely to be greatly influenced by the temperature of the heat exchange fluid. Therefore the exit of the temperature probe lumen is desirably as close to the balloon as possible to ensure that it is measuring the temperature of the blood in the IVC and not the femoral vein, or the introducer sheath, and yet far enough away from the balloon to  
5 accurately sense the temperature of the blood and not be unduly influenced by the temperature of the heat exchange fluid in the balloon. It has been found that if the probe lumen exit slot 30 is located about 0.5 cm or more proximal of the heat exchange region, this is generally acceptable. (The closeness of the probe tip to the expanded balloon also has the important advantage of allowing the balloon to somewhat act as a bumper to shield the tip of  
10 the probe from contacting the wall of the vessel.)

Likewise, the length that the probe extends from the exit opening in the lumen is important. Besides not prolapsing on the catheter shaft, it is important that the probe not extend far enough to lay against the balloon. Again, in this embodiment, it has been found  
15 that generally a gentle J shaped extension resulting in the thermistors being extended at least 1.8 mm from the shaft is desirable.

As can be seen in Figure 4, the end of the temperature probe lumen preferably includes a ramp 31 leading up to the opening. Thus, when the thermistor portion of the  
20 temperature control probe encounters the ramp, the ramp directs the thermistor up and through slot 30 into the blood stream. The end of the probe is generally shaped in a gentle J shape in a manner well known to those in the art of guide wires and like probes, and is constrained in a relatively straight shape within the temperature probe lumen. Once extended out of the lumen through the ramp, it assumes its substantially J-shape.

25 It will be appreciated that a J-shaped wire that is round may be rotated, and the distal tip of the probe may not be directed out away from the catheter. In order to assure proper orientation of the J tip away from the catheter, slot 30 is preferably in the form of a flat slot. The portion of temperature probe 20 that mates against this flat surface when the  
30 probe is extended is preferably in the form of a substantially flat probe. Thus, when the flat portion of the temperature probe encounters the flat ramp, the shape of the ramp orients the probe to ensure that the substantially J-shape extends outward away from the catheter shaft.

Accordingly, the catheter is inserted into a subject's blood vessel with the temperature probe retracted and the thermistors on the end of the probe within the temperature lumen in an undeployed state. By extending the temperature probe forward, the thermistor tip is moved through the slot and the temperature is thus deployed into the subject's blood stream.

Since the catheter is within a blood vessel, tip 40 of the thermistor preferably comprises an atraumatic tip. This helps prevent puncturing of the blood vessel or irritating the endothelium of the vessel if the temperature control probe encounters the wall of the blood vessel.

Other embodiments of an on-board temperature probe are clearly within the contemplation of this invention. With reference to Figure 3A, it can be seen that instead of having a lumen within the catheter for a movable temperature probe as shown in Figure 2A, a tube with a channel 50 may extend along the exterior of the catheter shaft. With the embodiment illustrated in Figure 3A, the deployable temperature probe may be deployed into its substantially J-shape through a slot as illustrated in Figure 3B.

Figures 5 illustrates alternative embodiment of the catheter system and the on-board temperature probe. The temperature probe 150 is fixedly contained within a temperature probe channel 152 and held in place by plug 154. The distal portion 156 of the temperature probe is upwardly biased so that if unrestrained it assumes a curved shape 156' with the tip extending outward away from the catheter body. A biodegradable band such as a suture 61 that may be rapidly dissolvable in blood restrains the distal portion against the shaft of the catheter. When the catheter is placed into the blood stream, the restraining band is dissolved and the distal portion of the probe assumes its curved configuration 156 with the temperature sensors in the tip 158' extending outward from the catheter shaft. Preferably this assumes a gentle J shape as described above to adequately locate the temperature sensor away from the catheter shaft but to have an atraumatic configuration. The distal portion of the probe may have a mechanical bias such as a fixed shape with spring-like bias, or it may have a temperature sensitive bias. That is, it may have a straight shape when at room temperature, but be made of a shape memory material such as nitinol or various temperature memory polymers, so it is straight at room temperature but assumes a curved shape when it is warmed to body temperature by the blood. If this type of shape memory material is used, a restraining

band need not be used, although it might also be used as an additional restraint. It should be noted that whenever a probe tip is described herein as biased in a particular configuration, that bias may be a permanent mechanical bias or it may be a bias that is temperature dependent as described herein, and both are within the contemplation of this invention.

5

Figure 6 illustrates another embodiment wherein the temperature probe is fixed in its axial orientation, and uses a "pull wire" mechanism to deploy the distal portion of the temperature probe away from the catheter shaft. In this embodiment, two wires 70, 71 are used to deploy the temperature probe into the bloodstream. The distal portion is configured, either as a spring (not illustrated) or a solid portion with cut-out sections. The wires are attached to the tip at a location slightly off-center. By pulling on one wire or the other, the top of the distal portion is compressed, and the lower portion expands to deploy the temperature probe into the bloodstream, preferably in a gentle, substantially J-shape. Reversing the process may return the probe to its generally straight configuration and thus minimize its profile for insertion and withdrawal. Various mechanism for activating the pull wire or pull wires are known in the art and are not illustrated here.

Another embodiment of an on-board, deployable probe is illustrated in Figures 8A and 8B. An outwardly biased member comprised of two legs 162, 164 which may be a unitary member is provided at an appropriate location proximal of the heat exchange region. The temperature sensor, such as a thermistor 166 is located in the central portion between the two legs, so that when they assume their outward configuration (Figure 8A) the temperature sensor is held outward away from the catheter shaft. In this embodiment, the legs may be rigid, for example a flat piece of plastic, and may be provided with a slot 168 in which to retract when compressed. In this Figure the slot is shown as provided for the forward leg, but it is equally acceptable for the forward leg to be fixed and the rear leg to retract when compressed. The upwardly biased member 162/164 may in fact be a curved member and not two distinct legs, as will be readily appreciated by those in the art. Alternatively, the upwardly biased member 162/164 may simply be compressible into a flat configuration and not a slidable configuration as illustrated.

10

The temperature sensor, such as thermistor 166, is attached to two signal carrying wires 170, 172 that carry the temperature sensing signal to the exterior plug 96. As stated previously, it is important that the wires be thermally insulated so that the temperature

sensed by the thermistor 166 is that of the blood flowing over it and is not a temperature of the catheter shaft conducted up the wires 170, 172.

The deployed sensor of this embodiment has the advantage that nothing need  
5 be done to deploy the on-board sensor. That is, it is essentially always deployed, but will compress down against the shaft upon insertion through an introducer sheath so that it assumes a small profile for insertion, but will immediately spring back out when unconstrained in the bloodstream.

10 Yet another embodiment is depicted in Figures 9A and 9B. In this embodiment, a movable temperature probe 178 with an upwardly biased distal portion 180 is placed in a temperature probe lumen with an open window 174 and a closed distal end 176. Prior to being deployed the distal end of the probe is retained within the distal end 176 of the lumen. When the probe is withdrawn a short distance (shown in Figure 9B) the upwardly  
15 biased portion exits through the window and assumes the curved configuration that orients the temperature sensor 182 away from the catheter shaft. When the catheter is subsequently withdrawn, the temperature probe will naturally fold down against the catheter shaft as it is being drawn through the introducer sheath.

20 Whenever the deployment of a temperature probe is accomplished by the axial movement of the probe, the amount of axial movement may be important in order to orient the temperature sensor the proper distance away from the catheter shaft. One method of doing so is shown in Figures 18A and 18B. An indicia, such as a marker band 184, may be located on the distal end of the temperature probe, and when that marker is at the proper  
25 location that would indicated the amount of axial movement of the temperature probe. In the example illustrated, the probe is deployed by withdrawing the temperature probe, and the amount of withdrawal necessary is indicated when the marker band just clears the exit port 86. Of course, the same effect may be had if the marker band is used to indicate the advancement of the temperature probe as in Figure 1; the marker would be placed farther up  
30 on the distal end of the probe and the correct amount of advancement indicated when the marker band is at the correct location relative to the exit port 86. The probe may then be locked in place in any of various means; for example affixing a keyed or barbed channel with a mating shape on the probe surface.



Other means of ensuring the correct amount of axial movement may be seen in Figures 10A and 10B and 17A and 17B. In 10A a temperature probe with a large distal portion is located in a temperature probe channel as in Figure 9A. The proximal end of the large distal portion of the temperature probe is too large a diameter to fit within the proximal temperature probe channel 188 and therefore when the temperature probe is withdrawn, it will only withdraw until the probe is withdrawn a certain distance. The probe distal portion then assumes its J shape, either because of its permanent bias or temperature based memory shape.

In this embodiment, the distal portion of the channel 188 must be large enough to accept the distal portion of the probe, yet the proximal portion of the channel 186 must be small enough not to accept the proximal end of that portion of the temperature probe. If the proximal portion of the probe tip is tapered or otherwise of increased diameter, a channel of the same diameter could be used for both sections which has obvious manufacturing advantages. Another way in which this could be accomplished as shown in Figs 17A and 17B. In this example, a section of enlarged diameter 190 is contained on the temperature probe in the section located in the window 174. When the probe is withdrawn, it can only be withdrawn until the enlarged section contacts the proximal edge of the window. In this way the exact amount of axial movement of the probe can be predetermined, and the exact shape of the distal portion determined for placement of the temperature sensor the appropriate distance from the catheter shaft.

Another embodiment for accomplishing this precise amount of axial movement is shown in Figures 16A and 16B. In this embodiment, the probe has a location of sharp increase in diameter 192, and the distal end of the temperature probe lumen has a flap 194 that is biased down against the catheter shaft. When the temperature probe is advanced it can exit under the flap 194, but when it is withdrawn, it cannot be withdrawn past the location of increased diameter. In this way the probe may be deployed forward, and then pulled back to the correct, predetermined position and no farther.

These methods of determining position of the probe after deployment may, of course, be used alone or in combination with each other.

Another embodiment of an on-board temperature sensor that has one diameter, for insertion for example, and another diameter where the temperature sensor is held away from the catheter shaft is depicted in Figures 13A, 13B and 14. In this embodiment, the temperature sensor 196, such as a thermistor is located on a balloon 202. Insulated wires 198, 199 conduct temperature signals from the thermistor outside the patient's body to a controller. An inflation channel 200 permits the introduction of inflation medium for example saline or CO<sub>2</sub> to inflate the balloon. The balloon may be, for example, a non-compliant PET balloon that has a predetermined shape and size. When fully inflated, this holds the temperature sensor a predetermined distance out into the bloodstream. This has the advantage of permitting some insulation, for example the use of an insulating inflation medium such as CO<sub>2</sub> and providing a very atraumatic means of locating the temperature sensor away from the catheter. The presence of the balloon just upstream of the heat exchange region may have an additional benefit of causing mixing eddies in the fluid stream (blood stream) that may further enhance heat exchange between the heat exchange region and the blood.

Two balloons may be provided as shown in Figure 15A and 15B. In Figure 15A each balloon 204, 206 is provided with a temperature sensor 208, 210. This may provide safety through redundancy or may provide for temperature measures at different locations. The two balloons may be located at different locations along a common lumen 212 and therefore the probe connecting wires 214, 216 for carrying the temperature signal may be located in the common lumen, and likewise the same lumen may serve as the inflation lumen for both balloons. Alternatively they may be independently controlled through independent inflation lumens.

In 15B, a temperature probe may be located on a wire, string, or other member 218 suspended between two balloons. This has the advantage of allowing the access to the temperature sensor from outside the catheter. In this situation it might be desirable to have the wires from the sensor travel outside the body through an external channel or not encased in a channel at all rather than locate them in the inflation channel.

Another embodiment is shown in Figure 11A and 11B. In this embodiment, a temperature probe 300 is in the form of a polyimide tube. The polyimide tube is contained in a temperature probe lumen 302. The lumen has a window 304 located at a location along the

catheter, for example about 3 cm proximal to a heat exchange balloon. The probe is fixed in the probe lumen proximal of the window by, for example, adhesive 303.

At the location of the window the polyimide tube is crimped 306. Near the  
5 location just proximal of the crimp, a thermister 308 is located in or on the tube. A second thermister 309 may be located just distal of the crimp to provide redundancy. Connector wire sets 314, 316 run from the thermisters to the plug the proximal end of the tube outside the patient's body.

The probe tube has two openings 318, 320 one on each side of the crimp. A  
10 pull wire 310 is affixed at the distal end 312 of the tube, and runs from that point of attachment inside the probe tube, out of the first opening 318, along the side of the probe tube, back into the tube through the second opening 320, and from there runs the length of the tube and is accessible to the operator at the proximal end (not shown).

In this embodiment, when undeployed, the temperature probe lies flat with  
15 sensors 308, 309 within the outer profile of the catheter and thus is insertable within any size introducer sheath that will suffice for the catheter. Once located in the desired location in the vasculature, the operator pulls the pull wire 310 which slides the distal portion of the probe tube backwards and causes the tube to bend at the crimp 306 and depoly the sensor through the window up and away from the catheter.

When the catheter is to be withdrawn, the pull wire may be pushed forward to  
20 once again cause the probe to lie flat in the probe lumen 302. In addition, the force of pulling the catheter back through the sheath can push in the deployed portion of the probe back down through the window and essentially return it to the undeployed position. Alternatively, or in addition, a biasing member such as a spring or elastomeric string 305 may attach the distal  
25 end of the tube 300 to a distal location in the probe lumen 302 so that the probe tube is pulled straight with the crimped portion within the window section of the tube unless the pull wire is withdrawn.

In this configuration, at the proximal end, a method of affixing the pull wire in  
the "pulled" configuration in a manner commonly known in the art, will allow the wire to be  
30 retracted, affixed in the retracted position which will fix the sensor in the deployed position. As discussed previously, methods of affixing the pull wire at a specific axial location will assure the proper amount of bending at the crimped location for proper deployment of the probe.

When the catheter is to be withdrawn, various devices for releasing the pull wire allow the catheter to be withdrawn with the probe in the undeployed configuration.

5 Similarly in Figure 12A and 12B an arm 222 hinged at an attachment to the catheter 224 may be raised away from the catheter body with a push wire, or relaxing of a restraining wire if the hinged arm has an upward bias.

Those skilled in the art will understand that other mechanisms and/or arrangements may be used to deploy the temperature probe into the bloodstream.

10

Although the present invention has been described with reference to specific exemplary embodiments, it will be appreciated that it is intended to cover all modifications and equivalents within the scope of the appended claims.

WHAT IS CLAIMED IS:

- 1                   1.     A catheter system for controlling the temperature of a patient, the  
2 catheter system comprising:  
  
3                   a catheter having a shaft and a heat exchange region;  
  
4                   an on-board temperature probe, said temperature probe having a temperature  
5 sensor and a signal carrying mechanism such that when said catheter is inserted into the body  
6 of a patient such that said heat exchange region is located inside the body of said patient, said  
7 signal carrying mechanism extending from said sensor to a location outside of the body of the  
8 patient;  
  
9                   said probe having an undeployed configuration and a deployed configuration,  
10 said probe movable between said undeployed configuration and said deployed configuration  
11 such that when the probe is in said deployed configuration, said sensor is located farther away  
12 from said catheter body than when said probe is in said undeployed configuration.
- 1                   2.     A catheter system in accordance with claim 1 wherein said probe is  
2 movable between said undeployed and said deployed configuration without any operator  
3 intervention.
- 1                   3.     A catheter system in accordance with claim 1 wherein said probe is  
2 movable between said undeployed and said deployed configuration by operator intervention.
- 1                   4.     A catheter system in accordance with claim 1 wherein said temperature  
2 sensor is a thermistor.
- 1                   5.     A catheter system in accordance with claim 1 wherein said temperature  
2 probe comprises a plurality of temperature sensors.
- 1                   6.     A catheter system in accordance with claim 1 wherein said temperature  
2 probe comprises shape memory material.
- 1                   7.     A catheter system in accordance with claim 6 wherein said temperature  
2 probe comprises nitinol.

1                   8.     A catheter system in accordance with claim 6 wherein said temperature  
2 probe comprises shape memory polymers.

1                   9.     A catheter system in accordance with claim 1, further comprising a  
2 controller, said temperature sensor generating a signal representing a sensed temperature, said  
3 signal carried from said sensor to said controller by said signal carrying mechanism, said  
4 controller controlling the heat exchanged between said heat exchange region and the blood of  
5 said patient in response to said signal.

1                   10.    A catheter system in accordance with claim 9 wherein said catheter  
2 system comprises a fluid flow heat exchange catheter having the temperature of said heat  
3 exchange region affected by flowing heat exchange fluid, said controller controlling the  
4 temperature of said heat exchange region by controlling the temperature of said heat  
5 exchange fluid.

1                   11.    A catheter system in accordance with claim 9 wherein said catheter  
2 system comprises a fluid flow heat exchange catheter having the temperature of said heat  
3 exchange region affected by flowing heat exchange fluid, said controller controlling the  
4 temperature of said heat exchange region by controlling the rate of flow of said heat  
5 exchange fluid.

1                   12.    A catheter system for sensing the temperature of a patient, the catheter  
2 system comprising:

3                         a catheter having a shaft and a heat exchange region;

4                         a temperature probe lumen, the lumen defining an aperture that is located  
5 proximal of the heat exchange region; and

6                         a deployable temperature probe, the temperature probe including a  
7 temperature sensor and a signal carrying mechanism that extends from the sensor to a  
8 location outside of the patient, the temperature probe having an undeployed configuration and  
9 a deployed configuration, the temperature probe being movable between the undeployed and  
10 deployed configurations;

11                    wherein when the temperature probe is in the deployed configuration, the  
12 temperature sensor is located further from the shaft than when the temperature probe is in the  
13 undeployed configuration; and

14                    wherein the temperature sensor generates a signal representing a sensed  
15 temperature and the signal carrying mechanism transmits the signal from the temperature  
16 sensor to the location outside the patient.

1                    13.     A catheter system in accordance with claim 12 wherein the  
2 temperature sensor comprises a thermistor.

1                    14.     A catheter in accordance with claim 13 wherein the temperature sensor  
2 comprises a second thermistor.

1                    15.     A catheter system in accordance with claim 12 wherein the catheter is  
2 a fluid flow heat exchange catheter whereby the temperature of the heat exchange region is  
3 controlled by a flow of heat exchange fluid.

1                    16.     A catheter system in accordance with claim 15 wherein the shaft  
2 includes fluid flow lumens for flow of heat exchange fluid to the heat exchange region.

1                    17.     A catheter system in accordance with claim 12 wherein the  
2 temperature probe is deployed by an operator.

1                    18.     A catheter system in accordance with claim 17 wherein the  
2 temperature probe is moved to the deployable configuration by removing a constraint that  
3 constrains the amount of movement of the temperature probe within the temperature probe  
4 lumen.

1                    19.     A catheter system in accordance with claim 17 wherein the  
2 temperature probe is deployed to the deployed configuration by at least one pull wire.

1                    20.     A catheter system in accordance with claim 17 wherein the  
2 temperature probe is in the from of a tube containing thermistor wires.

1                    21.     A catheter system in accordance with claim 12 wherein the  
2 temperature probe is automatically deployed between the undeployed configuration and the  
3 deployed configuration.

- 1                   22.    A catheter system in accordance with claim 21 wherein the  
2   temperature probe is heat activated.
- 1                   23.    A catheter system in accordance with claim 22 wherein the  
2   temperature probe comprises nitinol.
- 1                   24.    A catheter system in accordance with claim 21 wherein the  
2   temperature probe is spring activated.
- 1                   25.    A catheter system in accordance with claim 21 wherein the  
2   temperature probe includes a biodegradable restraining element.
- 1                   26.    A catheter system in accordance with claim 12 wherein the  
2   temperature probe lumen is within the catheter shaft and coupled thereto.
- 1                   27.    A catheter system in accordance with claim 12 wherein the  
2   temperature probe lumen is external to the catheter shaft and coupled thereto.
- 1                   28.    A catheter system in accordance with claim 27 wherein the  
2   temperature probe lumen extends along only a portion of the catheter shaft.
- 1                   29.    A catheter system in accordance with claim 27 wherein the  
2   temperature probe lumen extends along an entire length of an inserted portion of the catheter  
3   shaft.
- 1                   30.    A catheter system in accordance with claim 12 wherein the  
2   temperature probe lumen is incorporated within the catheter shaft and wherein the  
3   temperature probe lumen is extruded with the catheter shaft and is within the outer diameter  
4   of the shaft.
- 1                   31.    A catheter system in accordance with claim 12 wherein the aperture is  
2   located at a distal end of the temperature probe lumen.
- 1                   32.    A catheter system in accordance with claim 31 wherein the aperture  
2   comprises a ramp.
- 1                   33.    A catheter system in accordance with claim 32 wherein the ramp  
2   includes a shaped surface and the temperature probe includes a mating sensor.



1                   34.    A catheter system in accordance with claim 33 wherein the shaped  
2 surface is flat.

1                   35.    A catheter system in accordance with claim 12 wherein the sensor is in  
2 a range of 1.8 - 3.2 mm from the catheter shaft when the temperature probe is in the deployed  
3 configuration and is within the outer diameter of the catheter shaft when the temperature  
4 probe is in the undeployed configuration.

1                   36.    A catheter system in accordance with claim 12 further comprising a  
2 controller for receiving the signals from the signal carrying mechanism, the controller being  
3 configured to use the signals to control the body temperature of the patient by modifying the  
4 temperature of blood flowing within a blood vessel of the patient.

1                   37.    A catheter system in accordance with claim 12 wherein the catheter  
2 includes an atraumatic tip.

1                   38.    A catheter system for controlling the temperature of a patient, the  
2 catheter system comprising:

3                   a heat exchange catheter for placement in the flowing bloodstream of a  
4 patient, said catheter having a heat exchange region thereon;

5                   an on board temperature probe, said probe containing temperature sensors and  
6 signal carrying mechanisms, said signal carrying mechanisms extending from said sensors to  
7 a controller, said probe having an undeployed configuration and a deployed configuration, the  
8 temperature probe being movable between the undeployed and deployed configurations,  
9 wherein when the temperature probe is in the deployed configuration, the temperature sensor  
0 is located upstream in the bloodstream of the patient and further from the shaft than when the  
1 temperature probe is in the undeployed configuration;

2                   wherein the temperature sensor generates a signal representing a sensed  
3 temperature of the blood in the bloodstream, and the signal carrying mechanism transmits the  
4 signal from the temperature sensor to the controller; and

5                   said controller controls the temperature of said heat exchange region in  
6 response said signal.

1                   39.     A method of monitoring the body temperature of a patient by  
2     monitoring the temperature of blood flowing within a blood vessel of the patient, the method  
3     comprising:

4                   advancing a catheter body comprising a temperature probe lumen that extends  
5     along a catheter shaft and that includes an opening defined at a distal end portion into the  
6     patient's blood vessel such that the opening is in contact with the patient's blood; and

7                   deploying a temperature probe from within the temperature probe lumen such  
8     that a distal end portion of the deployable temperature probe protrudes through the opening  
9     into the blood flowing within the blood vessel.

1                   40.     A method in accordance with claim 39 wherein the deployable  
2     temperature probe comprises shape memory material at a tip portion at the distal end portion  
3     such that when it warms, it curves through the opening.

1                   41.     A method in accordance with claim 39 wherein the distal end of the  
2     temperature probe lumen includes a ramp coupled to the opening thereby guiding the distal  
3     end portion through the opening.

1                   42.     A method in accordance with claim 39 wherein the temperature sensed  
2     is venous blood.

1                   43.     A method in accordance with claim 41 wherein the blood vessel is the  
2     inferior vena cava.

1                   44.     A method in accordance with claim 41 wherein the blood vessel is the  
2     femoral vein.

1                   45.     A method of controlling the body temperature of a patient by  
2     monitoring the temperature of blood flowing within a blood vessel of the patient, the method  
3     comprising:

4                   advancing a catheter body comprising a temperature probe lumen that extends  
5     along a catheter shaft and that includes an opening defined at a distal portion of said lumen,  
6     said opening between said lumen and the patient's blood vessel such that the opening is in  
7     contact with the patient's blood;

8                   deploying a temperature probe, said temperature probe having a temperature  
9   sensor, from within the temperature probe lumen such that said temperature sensors  
10 protrudes through the opening into the blood flowing within the blood vessel;  
  
11                   generating a signal from said temperature sensor representing the temperature  
12 of the blood; and  
  
13                   providing said signal to a controller.

1                   46.   A method in accordance with claim 45 wherein the distal end of the  
2 temperature probe lumen includes a ramp coupled to the opening thereby guiding the distal  
3 end portion through the opening.

1                   47.   A method in accordance with claim 45 wherein the catheter includes a  
2 heat exchange region and the temperature of said heat exchange region is controlled by  
3 flowing fluid between the controller and the heat exchange region.

1                   48.   A method in accordance with claim 46 wherein the controller controls  
2 at least one of a temperature of the heat exchange fluid and a rate of fluid flow of the heat  
3 exchange fluid.

1                   49. A system for controlling the temperature of at least a portion of the  
2 body of a human or veterinary patient, said system comprising:  
3                   an elongate catheter that is insertable into the vasculature of the patient;  
4                   a heat exchanger at a first location on the catheter, a heat exchange fluid being  
5 passable through the catheter and through the heat exchanger such that heat will be  
6 exchanged between the heat exchange fluid flowing through the heat exchanger and blood  
7 flowing through the patient's vasculature in heat exchange proximity to the heat exchanger;  
8                   a temperature sensor at a second location on the catheter, said temperature sensor  
9 being initially disposable in a non-deployed position and subsequently disposable in a  
10 deployed position, said temperature sensor being operative, when in its deployed position, to  
11 sense the temperature of blood flowing through the patient's vasculature without substantial  
12 interference from heat exchange fluid passing through the catheter; and,  
13                   a controller which receives a temperature signal from the temperature sensor and, in  
14 response to such received signal, controls the temperature and/or rate of heat exchange fluid  
15 passing through the heat exchanger to cause heating or cooling of the patient's blood until the  
16 temperature sensed by the temperature sensor is substantially the same as a predetermined  
17 target temperature.

1                   50. A system according to Claim 49 wherein the temperature sensor  
2 comprises a thermistor.

1                   51. A system according to Claim 49 wherein the temperature sensor  
2 comprises at least first and second thermistors.

1                   52. A system according to Claim 49 wherein the catheter comprises a shaft  
2 having lumens through which heat exchange fluid flows to and from the heat exchanger.

1                   53. A system according to Claim 49 further comprising a deployment  
2 triggering apparatus whereby an operator may volitionally cause the temperature probe to  
3 move from its non-deployed position to its deployed position.

1                   54. A system according to Claim 53 wherein the deployment triggering  
2 apparatus comprises a movable constraining member which is initially disposed in a first  
3 position whereby it holds the temperature sensor in its non-deployed position and is

4 subsequently moveable to a second position whereby it no longer constrains the temperature  
5 sensor, thereby allowing the temperature sensor to move to its deployed position.

1           55. A system according to Claim 53 wherein the wherein the deployment  
2 triggering apparatus comprises at least one pull wire which, when pulled by an operator,  
3 causes the temperature sensor to move from its non-deployed position to its deployed  
4 position.

1           56. A system according to Claim 49 wherein the temperature sensor  
2 comprises a tube which contains thermistor wires.

1           57. A system according to Claim 49 further comprising an automatic  
2 sensor deployment apparatus whereby the temperature probe is automatically deployed from  
3 its non-deployed position to its deployed position.

1           58. A system according to Claim 57 wherein the automatic sensor  
2 deployment apparatus comprises a shape memory material which moves the temperature  
3 sensor from its non-deployed position to its deployed position as the shape memory material  
4 warms to the patient's body temperature following insertion of the catheter into the  
5 vasculature.

1           59. A system according to Claim 58 wherein the shape memory material  
2 comprises a Nichol-Titanium alloy.

1           60. A system according to Claim 57 wherein the automatic sensor  
2 deployment apparatus comprises a spring.

1           61. A system according to Claim 49 wherein the automatic sensor  
2 deployment apparatus comprises a biodegradable anchor which initially holds the  
3 temperature sensor in its non-deployed position and which subsequently biodegrades  
4 following insertion of the catheter into the vasculature, thereby allowing the temperature  
5 sensor to move to its deployed position.

1           62. A system according to Claim 49 wherein the catheter comprises an  
2 elongate shaft and the temperature sensor is connected to the controller by way of a wire  
3 which extends through the catheter shaft proximal to the temperature sensor.

1           63.    A system according to Claim 49 wherein the catheter comprises an  
2 elongate shaft and the temperature sensor is connected to the controller by way of a wire  
3 which extends outside of the catheter shaft proximal to the temperature sensor.

1           64.    A system according to Claim 63 wherein the wire is housed within a  
2 luminal member that is affixed to the catheter shaft proximal to the temperature sensor.

1           65.    A system according to Claim 49 wherein the catheter comprises a  
2 lumen which extends through at least the portion of the catheter proximal to the second  
3 location and wherein the temperature sensor may be advanced through said lumen and to its  
4 deployed position after the catheter has been inserted into the patient's vasculature.

1           66.    A system according to Claim 65 wherein an aperture is formed at the  
2 second location in communication with the lumen such that the temperature sensor may be  
3 advanced through the lumen and out of the aperture to a deployed position that is a spaced  
4 distance away from the catheter.

1           67.    A system according to Claim 65 wherein the lumen further comprises a  
2 ramp which deflects the temperature sensor out of said aperture.


1           68.    A system according to Claim 67 wherein the ramp includes a first  
2 shaped surface and the temperature sensor includes a second shaped surface which mates  
3 with the first shaped surface.


1           69.    A system according to Claim 68 wherein at least the first shaped  
2 surface is flat.

1           70.    A system according to Claim 49 wherein the temperature sensor, when  
2 in its deployed position, extends 1.8 - 3.2 mm away from the catheter.


1           71.    A system according to Claim 49 wherein the catheter includes an  
2 atraumatic tip.

Fig. 1

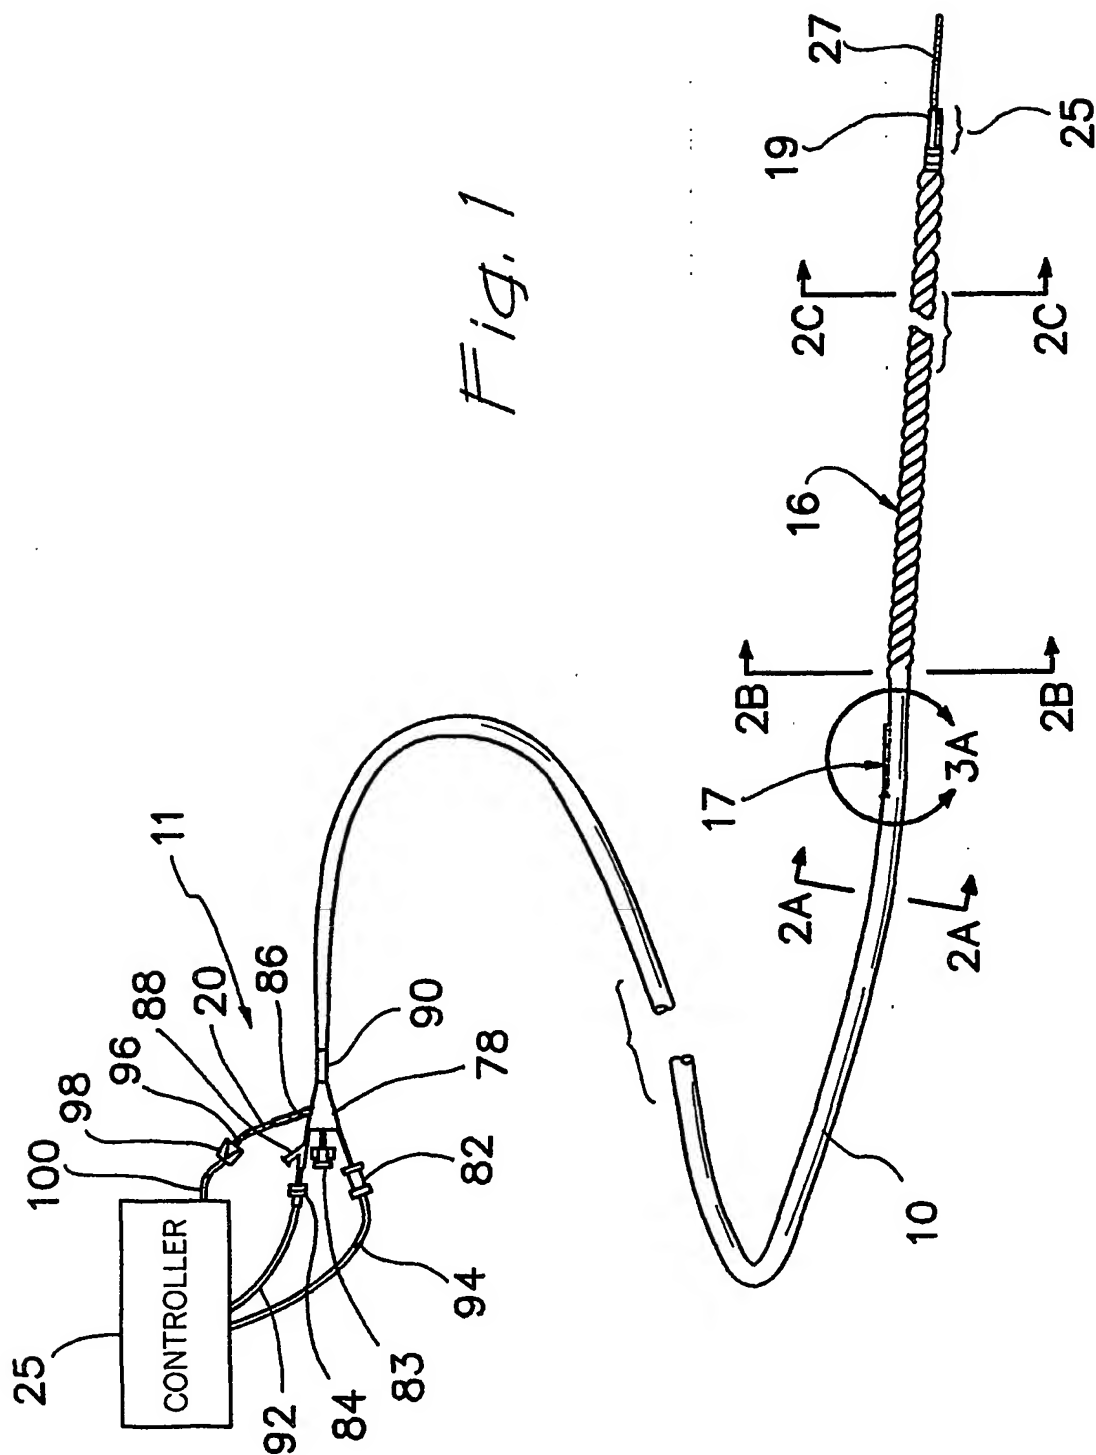


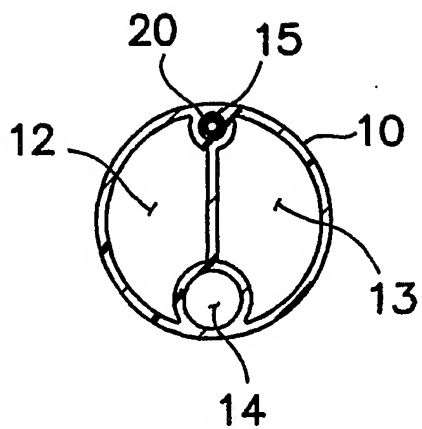


*Fig. 2A*

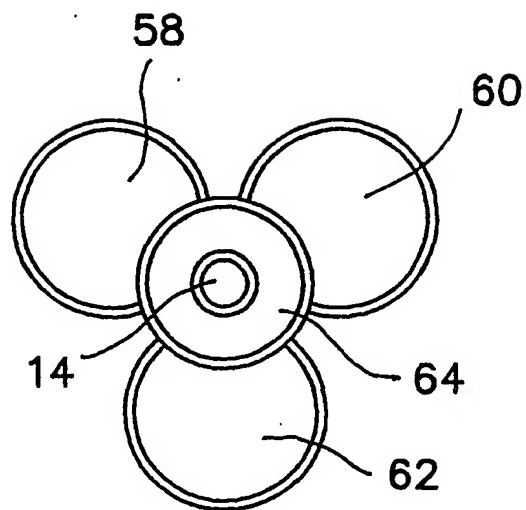

*Fig. 2c*



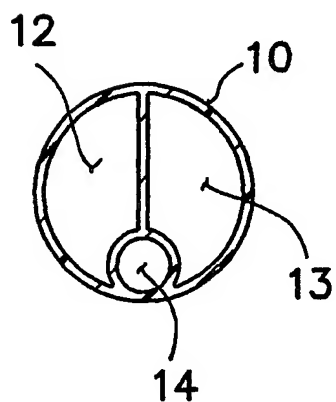


*Fig. 2B*


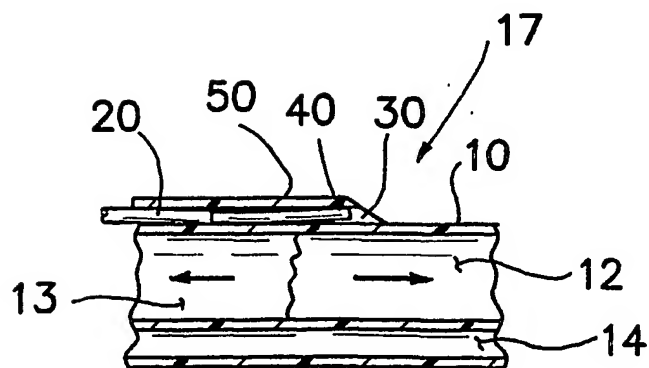



*Fig. 3A*



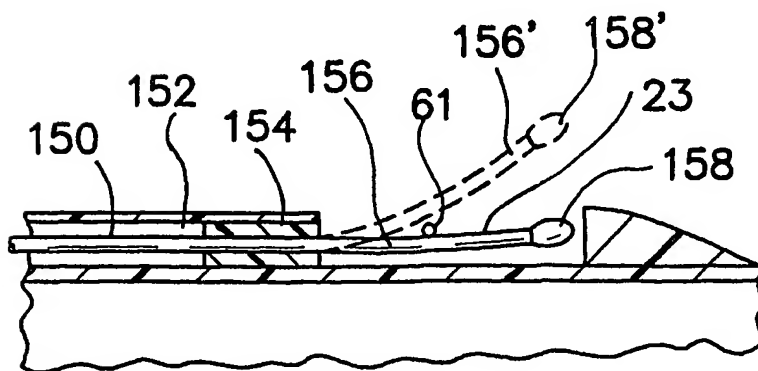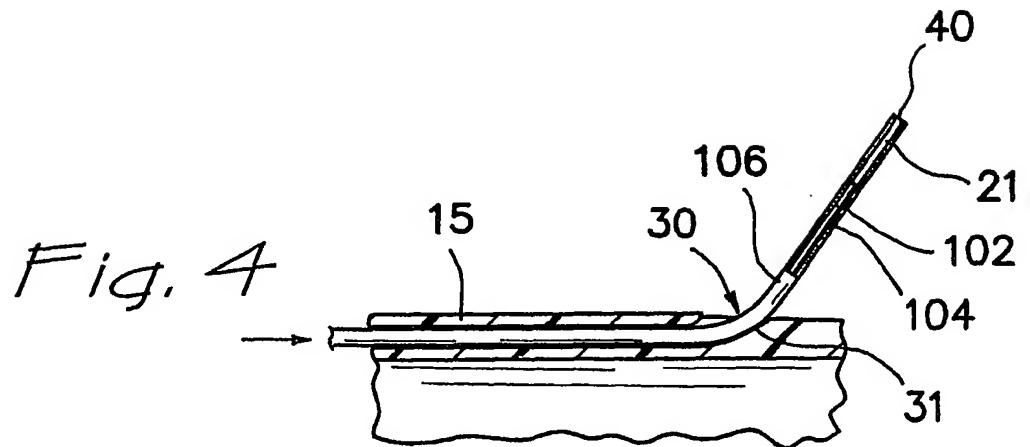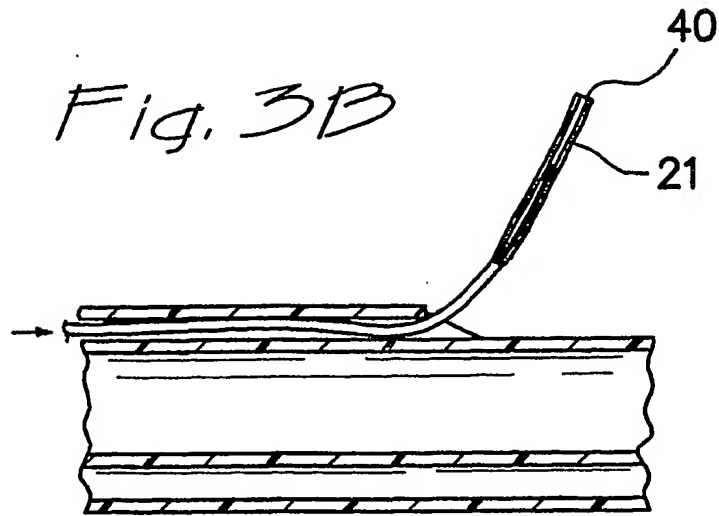


*Fig. 5*



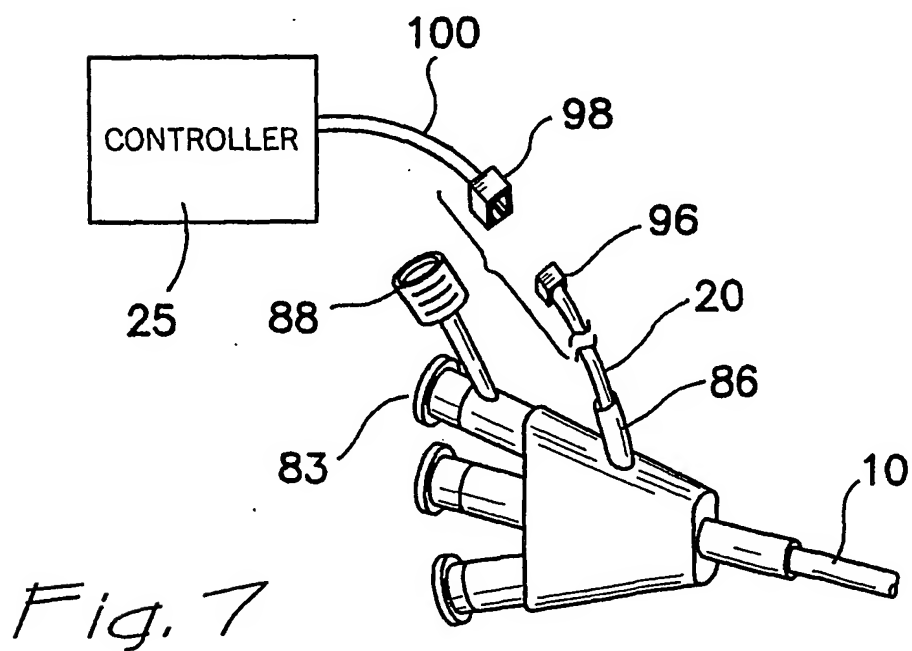
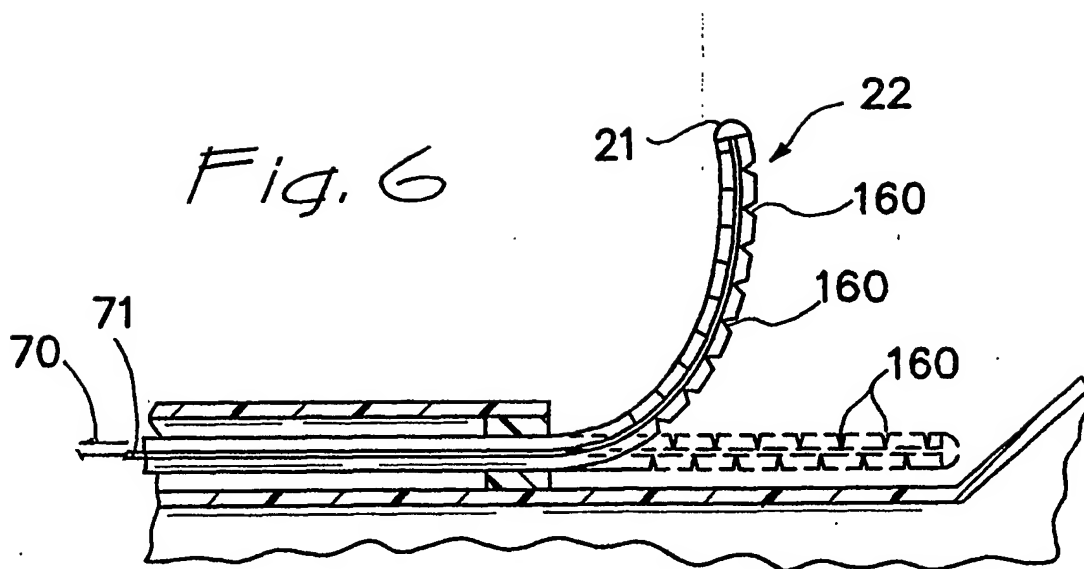



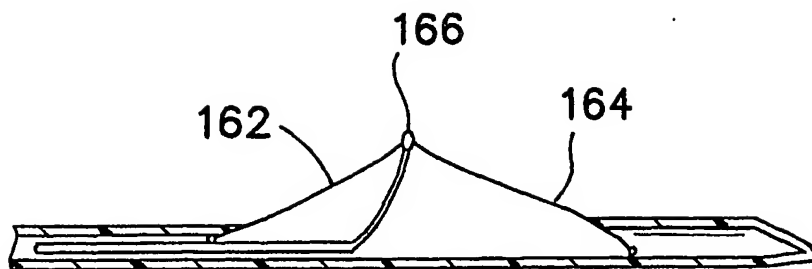



*Fig. 8A*

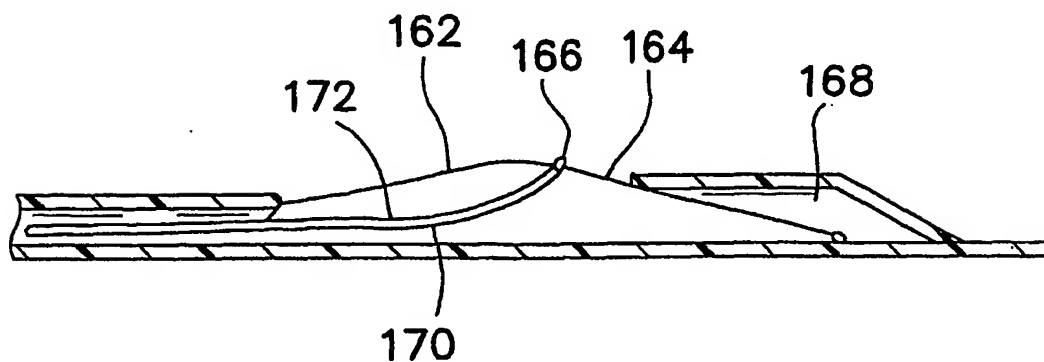


*Fig. 8B*

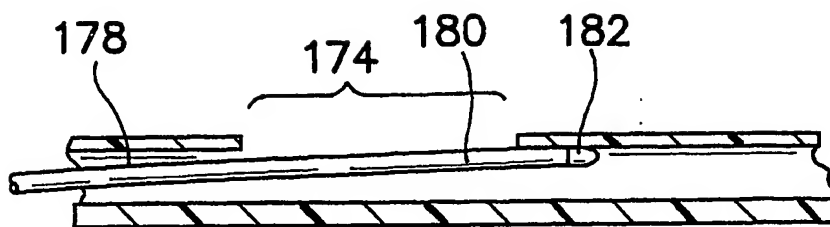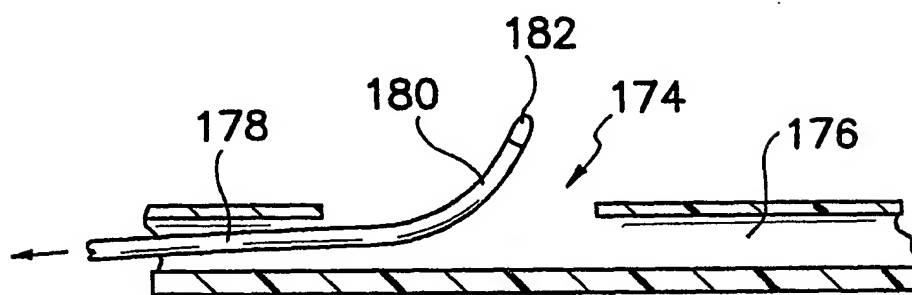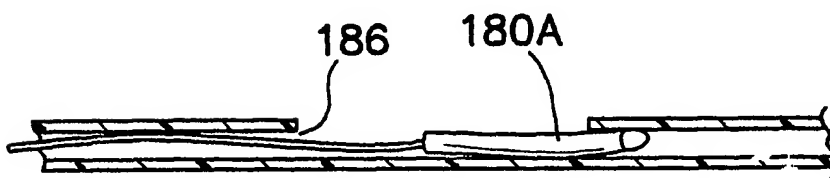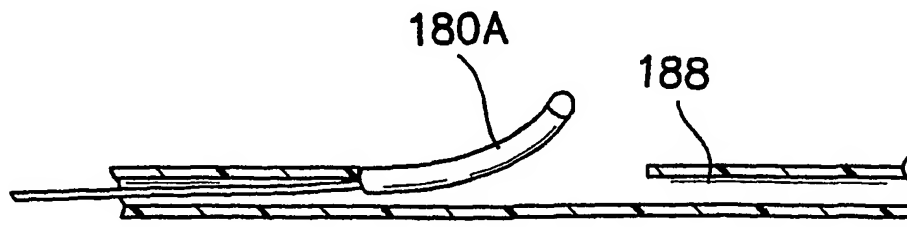*Fig. 9A**Fig. 9B**Fig. 10A**Fig. 10B*

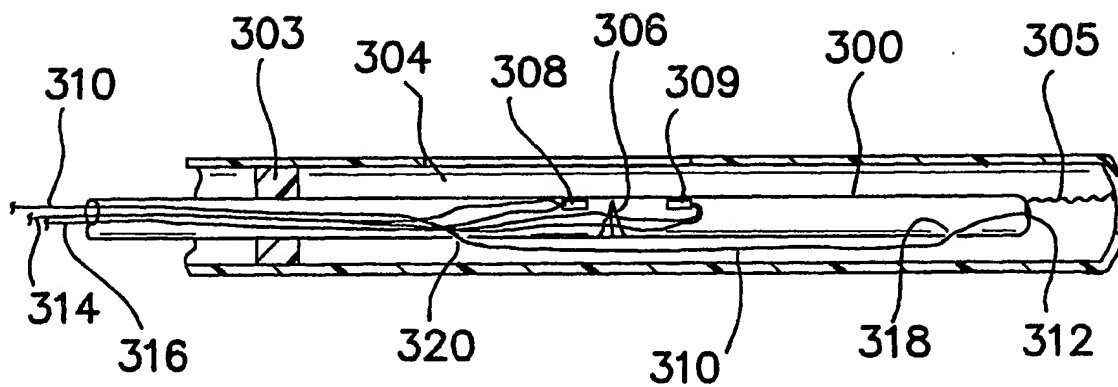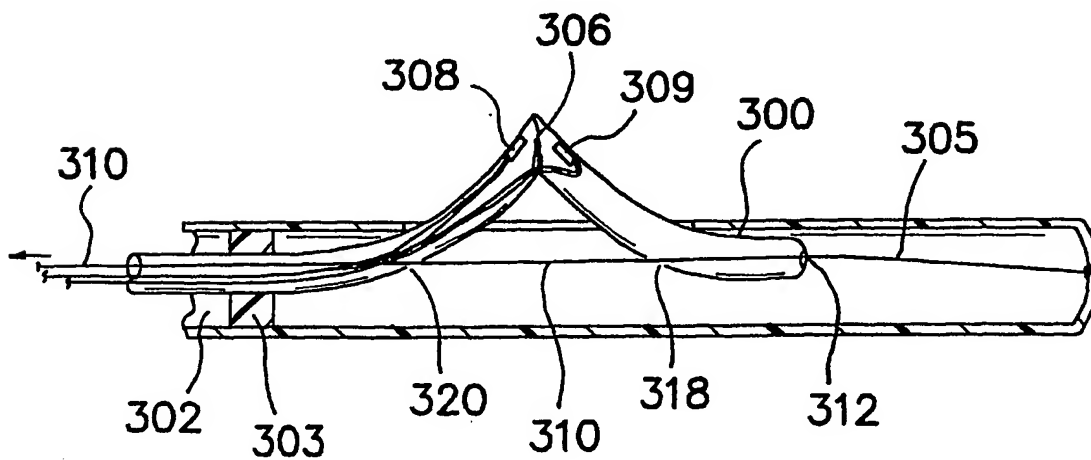
*Fig. 11A**Fig. 11B*

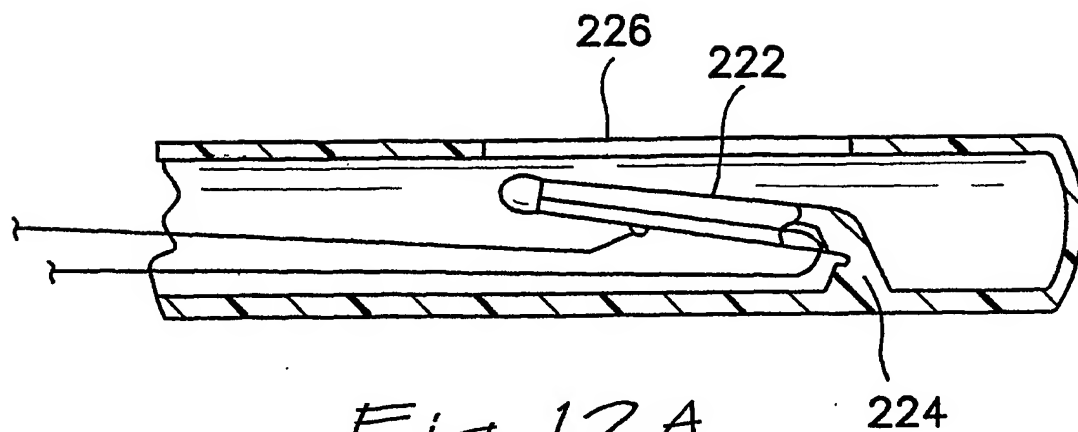


*Fig. 12A*

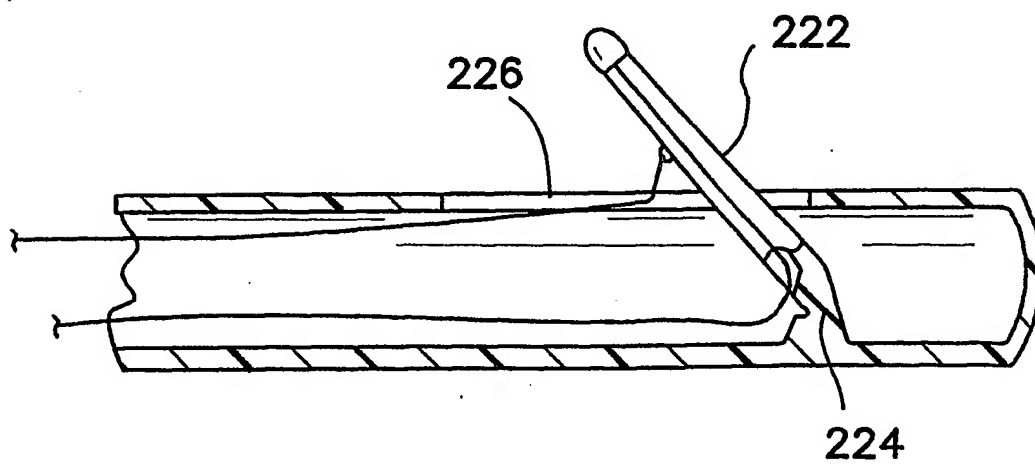


*Fig. 12B*

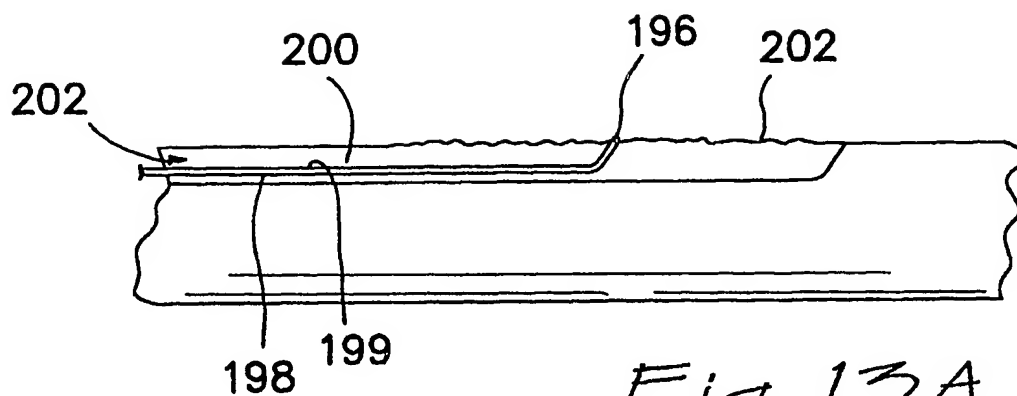





*Fig. 13A*

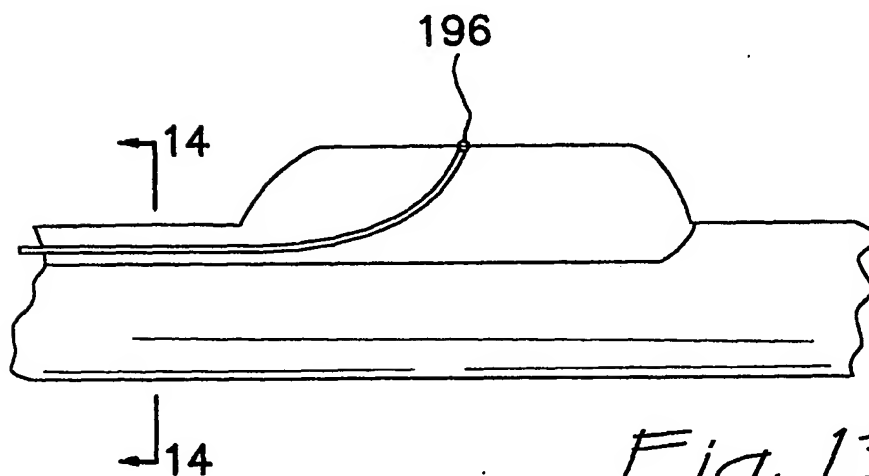


*Fig. 13B*

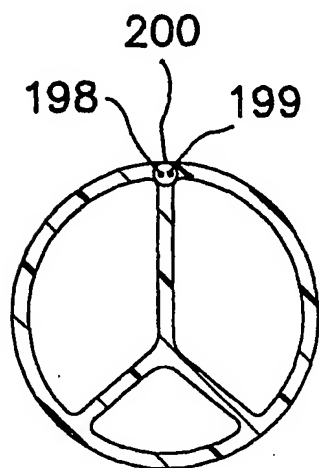


*Fig. 14*

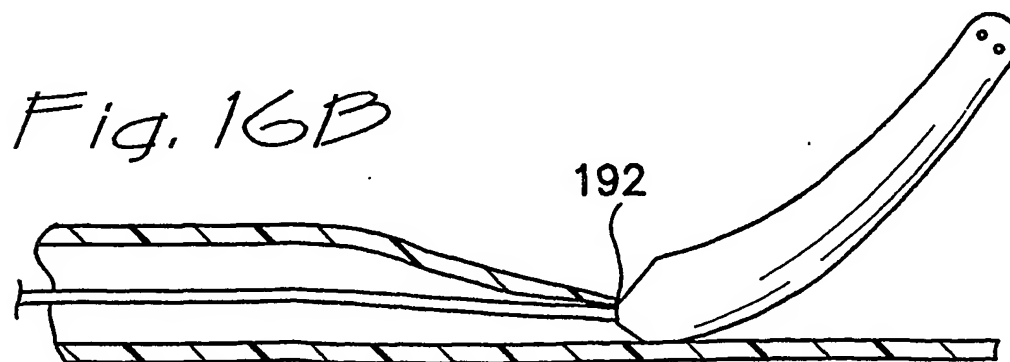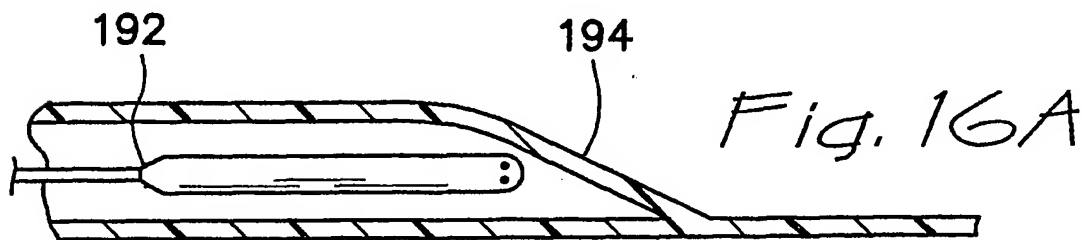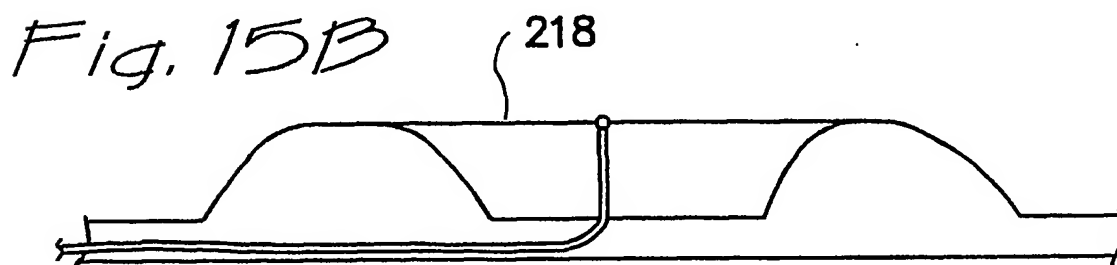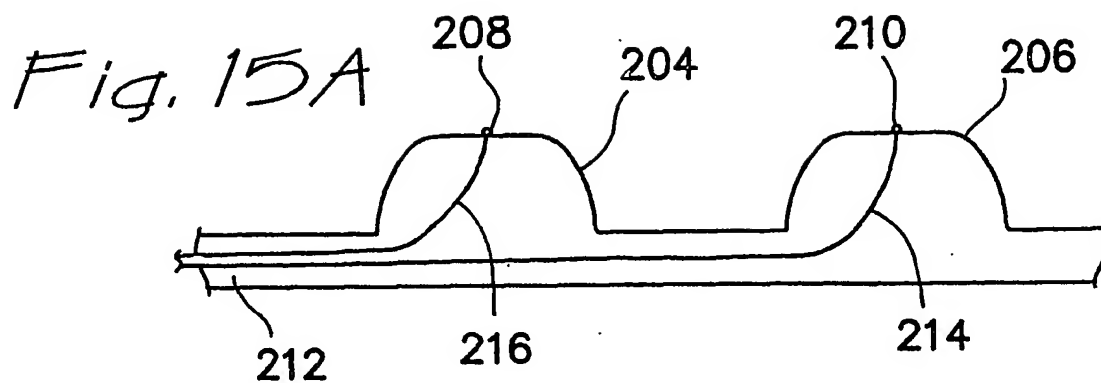




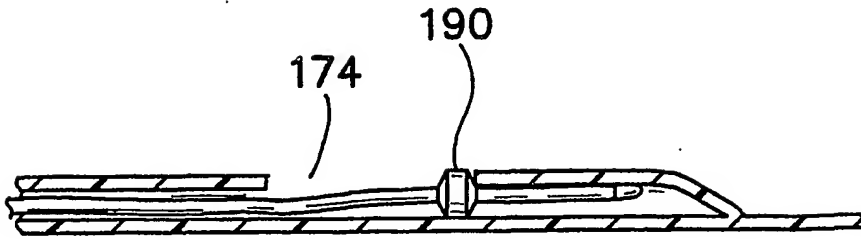


*Fig. 17A*

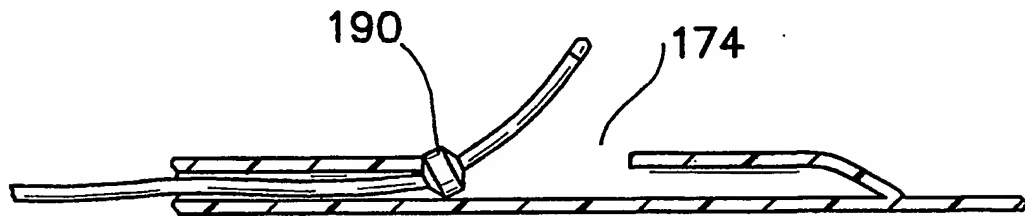

*Fig. 17B*

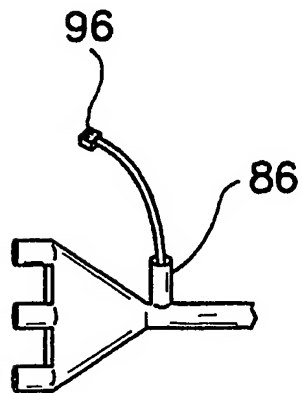

*Fig. 18A*

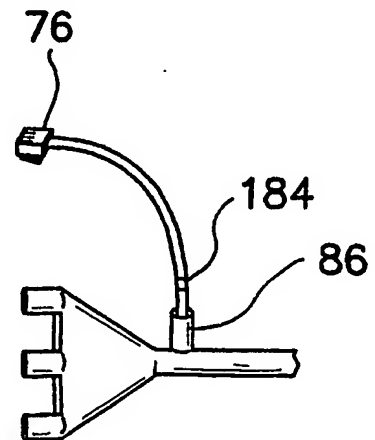

*Fig. 18B*

**This Page is Inserted by IFW Indexing and Scanning  
Operations and is not part of the Official Record**

**BEST AVAILABLE IMAGES**

Defective images within this document are accurate representations of the original documents submitted by the applicant.

Defects in the images include but are not limited to the items checked:

- ☒ BLACK BORDERS
- ☐ IMAGE CUT OFF AT TOP, BOTTOM OR SIDES
- ☐ FADED TEXT OR DRAWING
- ☐ BLURRED OR ILLEGIBLE TEXT OR DRAWING
- ☐ SKEWED/SLANTED IMAGES
- ☐ COLOR OR BLACK AND WHITE PHOTOGRAPHS
- ☐ GRAY SCALE DOCUMENTS
- ☐ LINES OR MARKS ON ORIGINAL DOCUMENT
- ☐ REFERENCE(S) OR EXHIBIT(S) SUBMITTED ARE POOR QUALITY
- ☐ OTHER: \_\_\_\_\_

**IMAGES ARE BEST AVAILABLE COPY.**

**As rescanning these documents will not correct the image problems checked, please do not report these problems to the IFW Image Problem Mailbox.**